

14
10
30
32
12
20
34

FIG 1



20

12

FIG. 2

Output of light to tissue
plus collection of light
from reflection

Input of light
for measurement

Returned light from
tissue to meter

18 20 22 26

FIG. 3


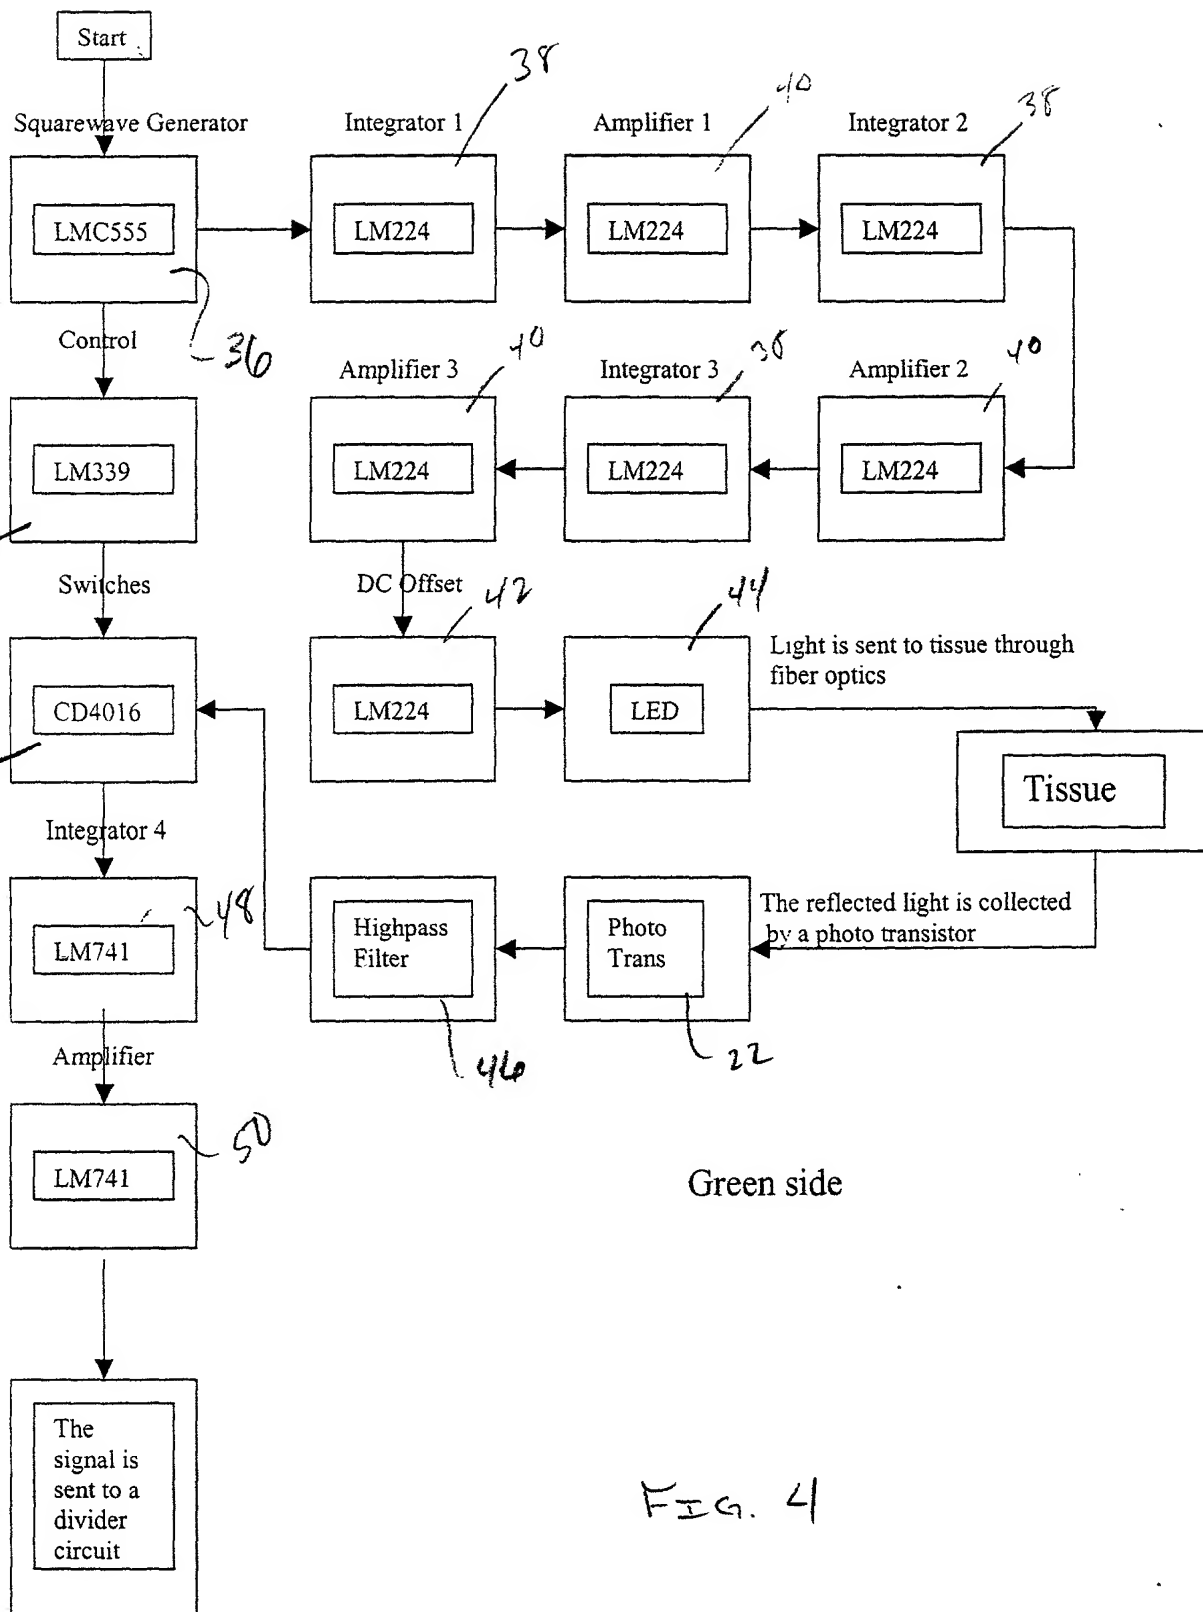


FIG. 4

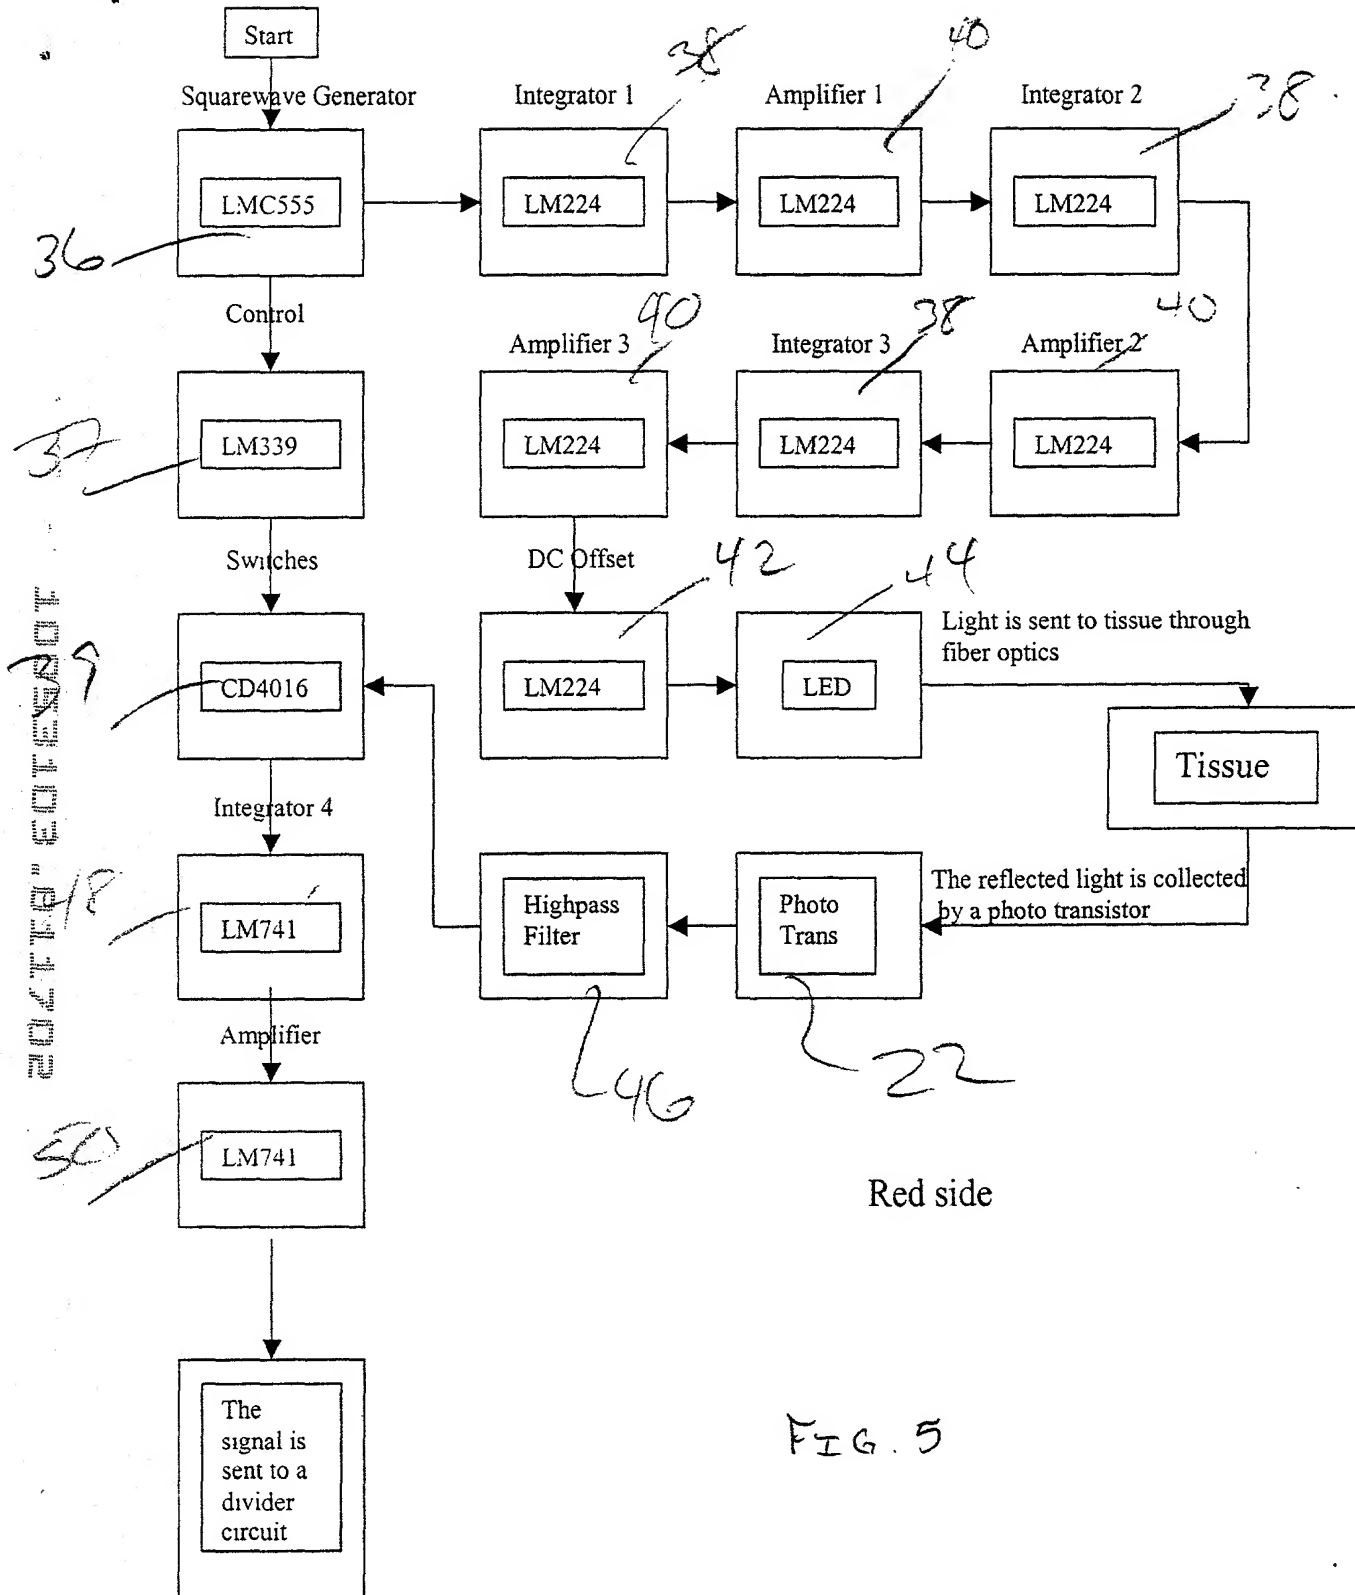

202503103.011702


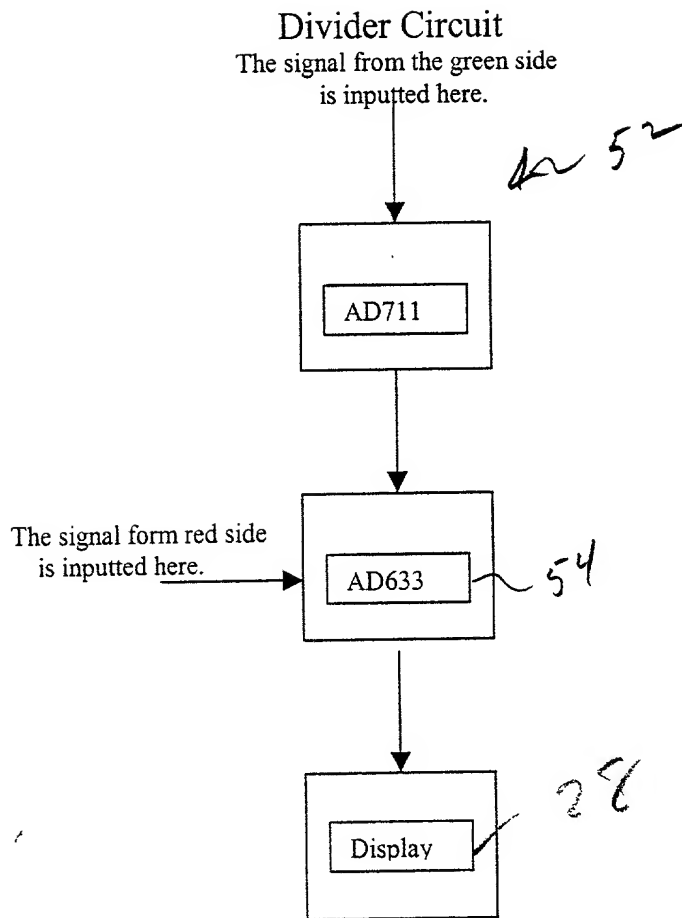


FIG. 6

2024TFO" EOTEE500T

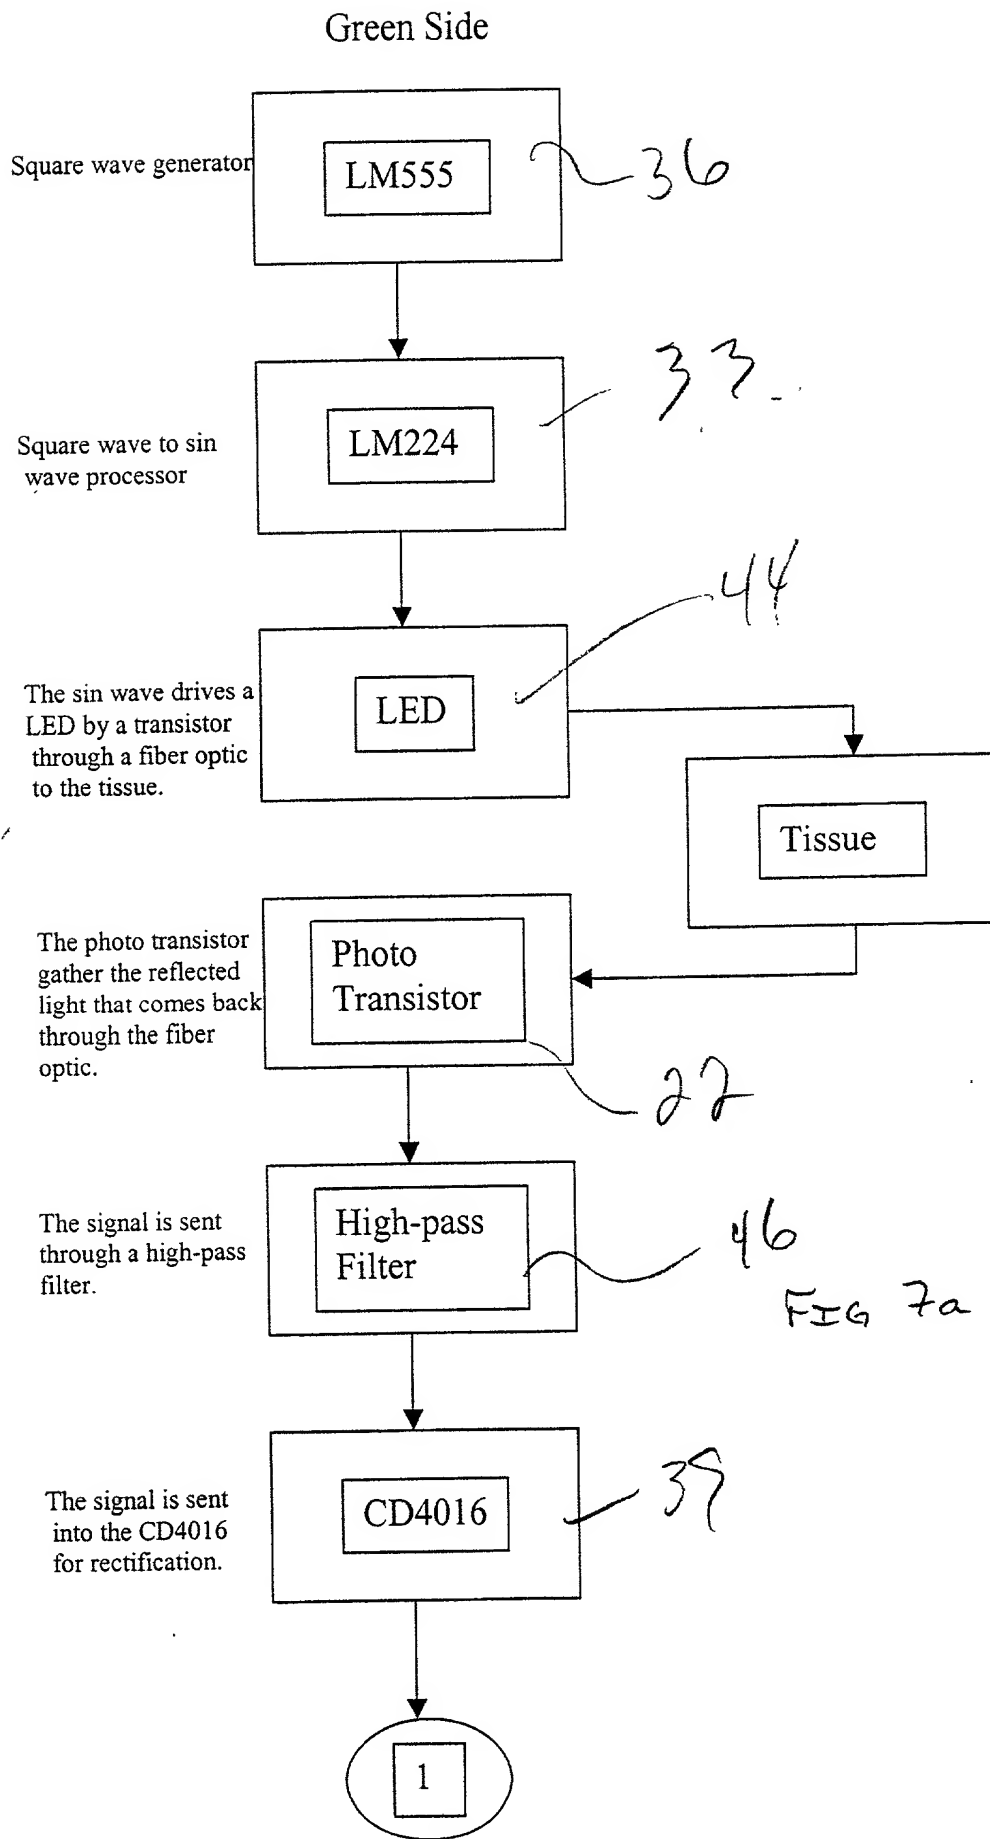

2025-10-01 14:00:00

Here the signal is
integrated and
amplified.


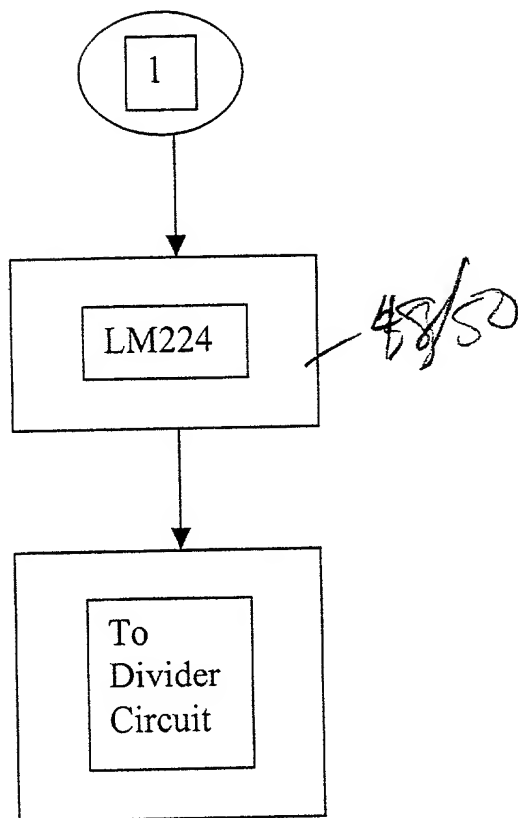



FIG. 7b

202503103-011702

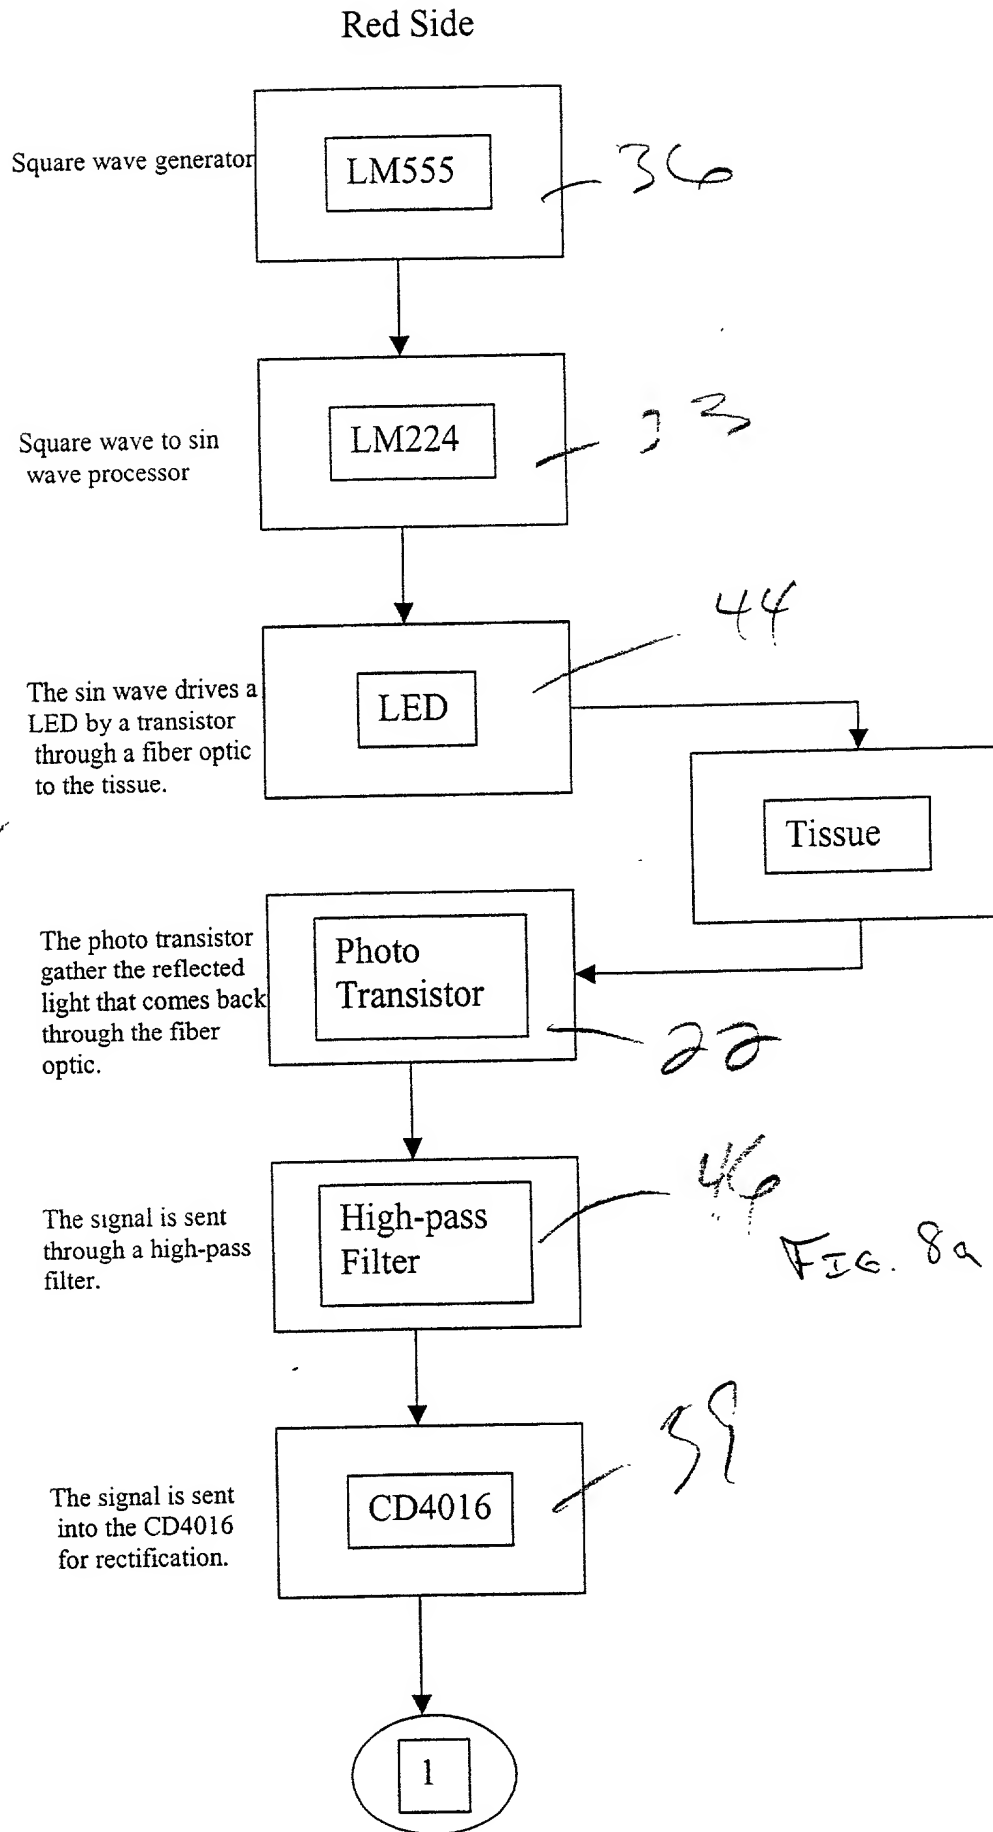

10053103.011702

Here the signal is
integrated and
amplified.

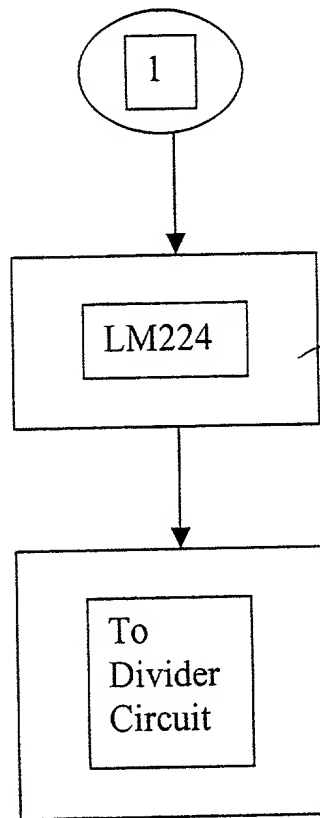

48/50

FIG. 8b

Divider Circuit

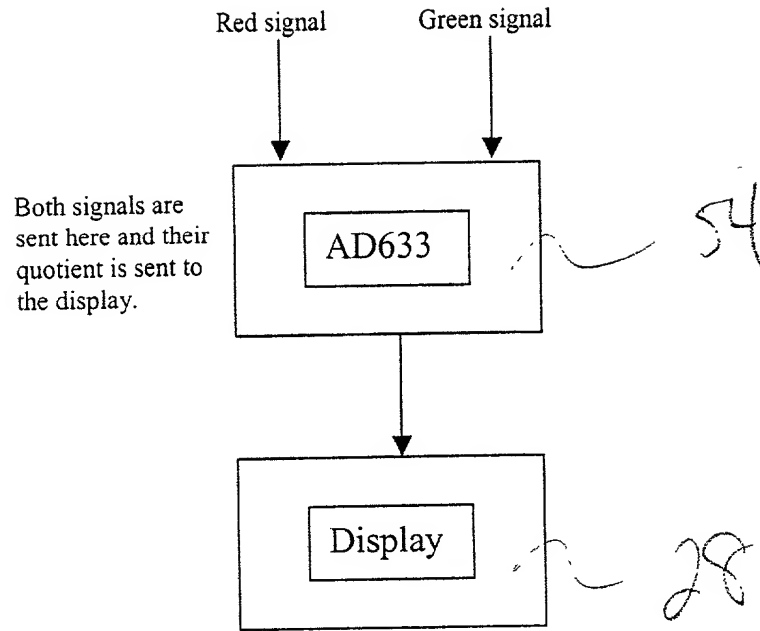


FIG. 9